



OR 4Vet

Multimodal diagnostic imaging
that inspires.

Medici DR Dental System

CMOS dental detector Pluto Size 2

High image quality & ease of use for your veterinary practice



 OR Technology

The expert by your side.

CMOS dental detector Pluto Size 2

The Pluto Size 2 is a digital intraoral sensor and has a CMOS sensor with a resolution of 20 μm . The sensor's CsI scintillator ensures optimal resolution. The sensor is an easy-to-use X-ray detector with cable and is dust and waterproof (comparable to IP68).

The Pluto Size 2 has an ergonomic design with smooth edges, rounded corners and a flexible cable for maximum patient comfort.


An easy-to-use high-speed USB interface allows easy connection to a PC without the need for an additional control unit.

- CMOS detector technology
- Low dose clinical imaging
- High resolution of 20 μm
- Wide dynamic range
- Slim, rounded corners and smooth edges
- Direct USB connectivity
- AED trigger, quick and easy workflow
- Durable materials and components
- Effective Imaging Area: 36 mm x 26 mm

Parameter

Sensor	
Detector Technology	CMOS
Scintillator	Directly deposited CsI:TI
Sensor size	40 mm x 31 mm x 4.5 mm
Effective Imaging Area	36 mm x 26 mm
Image Matrix	1800 x 1300 pixels
Pixel Pitch	20 μm
AD Conversion	16 bit
Spatial resolution	16 lp/mm
Ingress Protection	IP68 (the highest point of enclosures with a height greater than 1000mm below the surface of water, and the duration of the test is more than 30 minutes)
Sensitivity	>40 lsb/uGy
Trigger sensitivity	<100 uGy/s
Max linearity dose	>300 uGy
Length of cable	2.8m + - 50mm
Interface	USB 2.0
Power	<2W

Environmental	
Operating Temperature	10~35 °C
Storage & Transport Temperature	-10 to 55 °C
Operating Humidity	20~90% RH
Storage & Transport Humidity	10~95% RH
Operating Atmospheric Pressure	70 to 1060 kPa
Storage & Transport Atmospheric	70 to 1060 kPa

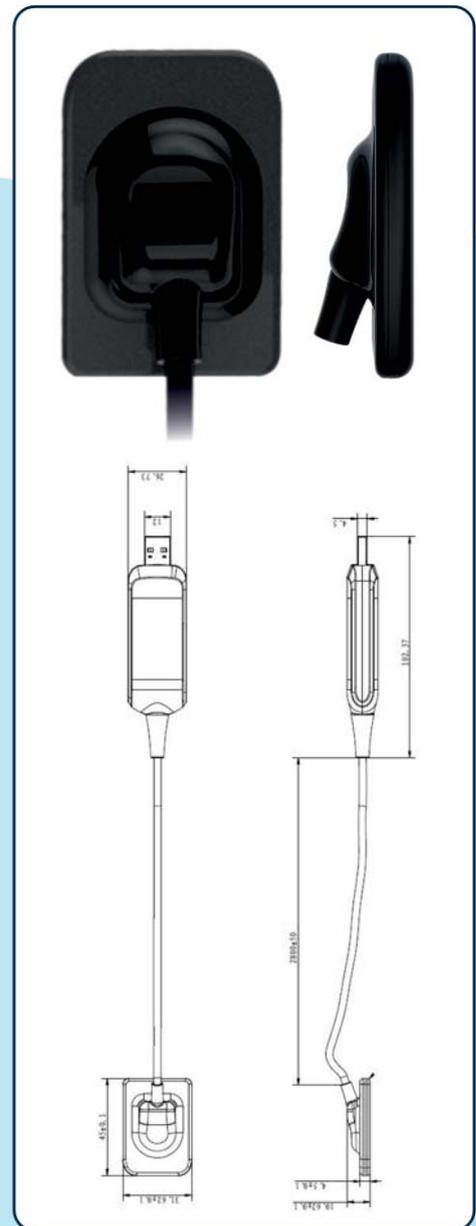

Specifications subject to revision without notice

The editor strives to impart correct and up to date information. The provided specifications are based on current knowledge and are subject to revision without notice. This brochure is subject to correction. The editor assumes no responsibility for the information being up to date, correct and complete. All furnished logos, pictures and graphics are property of the particular company and subject to copyright of the licensor. Use, dissemination, distribution or copying of the pictures, logos or text compiled or processed by the editor is subject to our written consent. All rights reserved.